


TRACEABILITY CHART

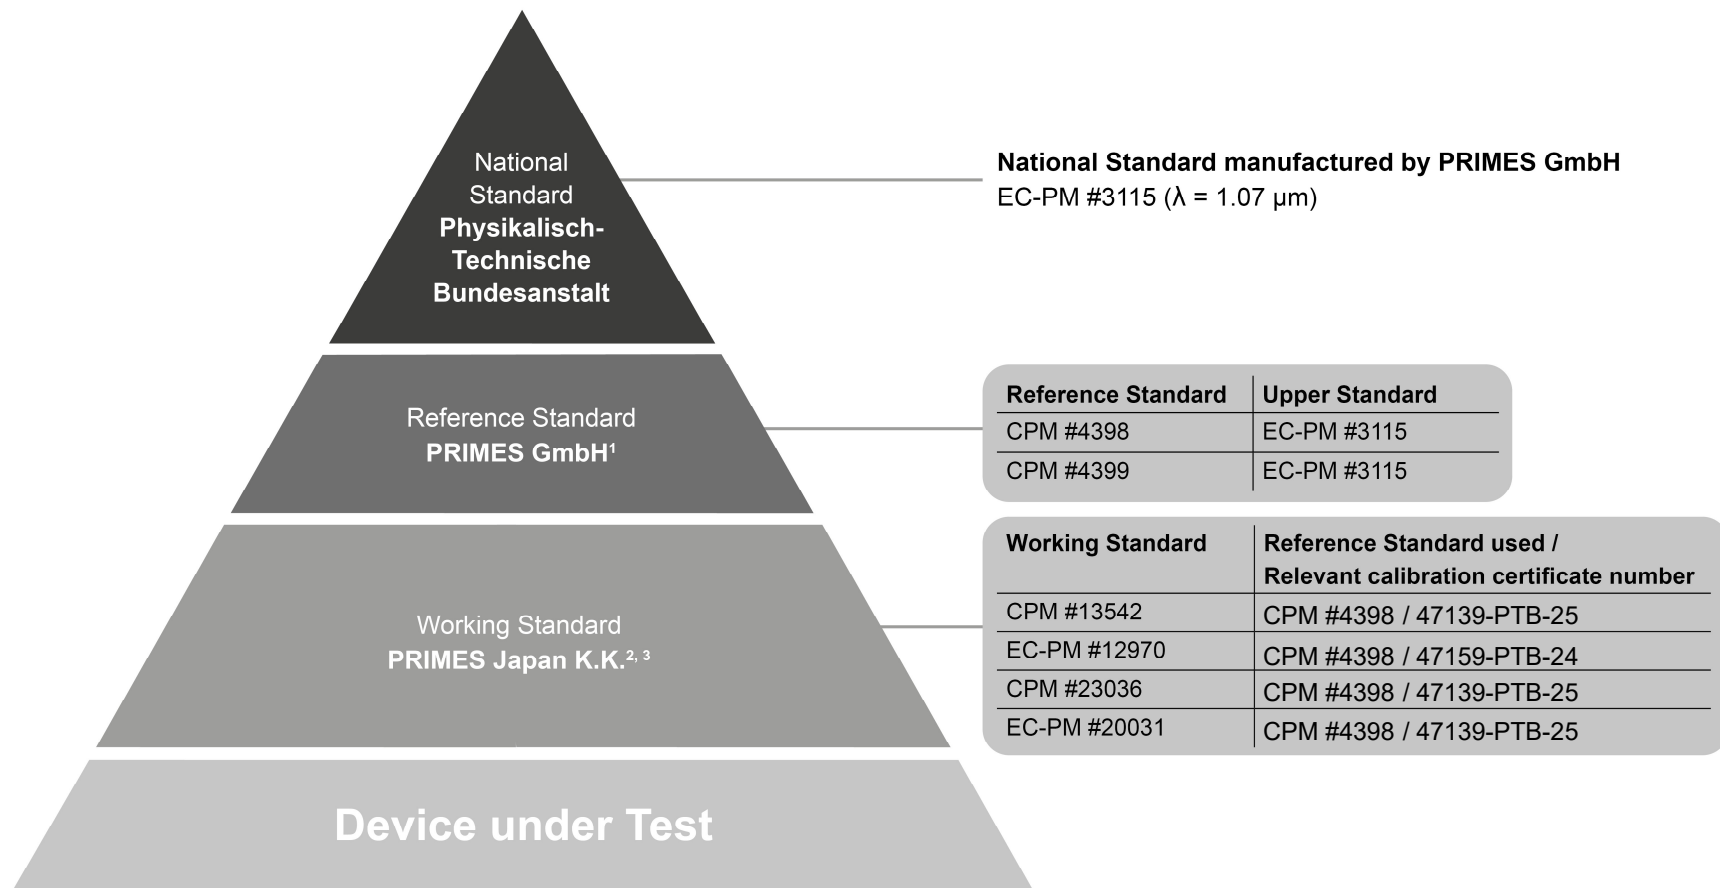

- 1) All reference standards are recalibrated once a year.
- 2) The working standards are recalibrated against the reference standards at least once every twentyfour months and compared against each other at least once every three months.
- 3) The working standards can be used continuously for up to twentyfour months, even if the traceable reference standard has been recalibrated against an upper standard in the meantime.